

Analyte Specifications:

Catalog Number:

**CCL11  
(Eotaxin)**


**92010**

**MultiCyt™ QBeads™ PlexScreen**


Reconstituting the Eotaxin standard in 2 mL of assay diluent results in a concentration of 5000 pg/mL. Standard curves for no-wash and 1-wash protocols were performed in triplicate (+/- S.D.). The limit of detection (dashed line) is 3 standard deviations above the mean of samples without Standard (N=12). Results are typical and may vary based on specific assay conditions.

### STANDARD CURVES

**No-Wash Assay Performance**

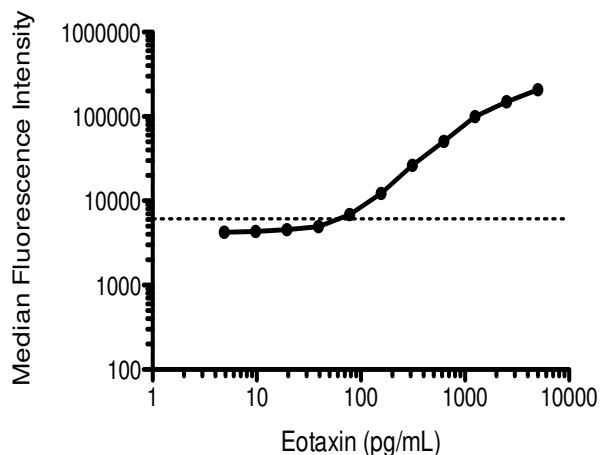

**1-Wash Assay Performance**

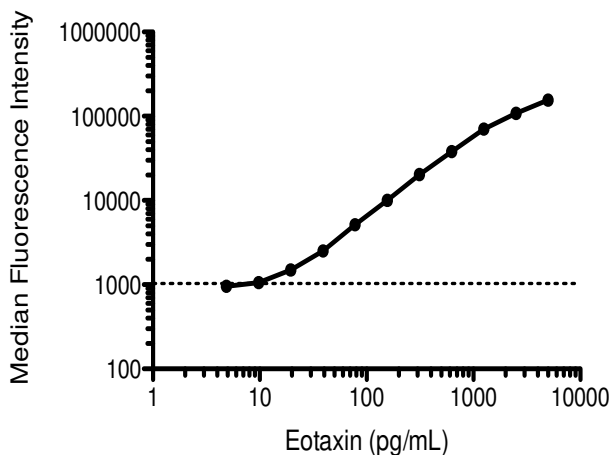

**Lowest Detectable Test Conc. (pg/mL): 78.1**

**Lowest Detectable Test Conc. (pg/mL): 9.8**

For research purposes only. Not for resale.

Rev. 1 Jan 2014