

Analyte Specifications:

Catalog Number:

VEGF


92049

MultiCyt™ QBeads™ PlexScreen


Reconstituting the VEGF standard in 2 mL of assay diluent results in a concentration of 5,000 pg/mL. Standard curves for no-wash and wash protocols were run in triplicate (+/- S.D.). The limit of detection, represented by the dashed line, is determined by adding 3 standard deviations to the mean of samples without VEGF (N=12). Results are typical and may vary based on specific assay conditions.

STANDARD CURVES

No Wash Protocol

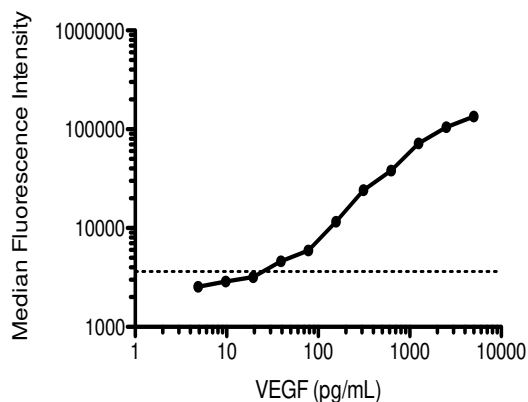

1-Wash Protocol

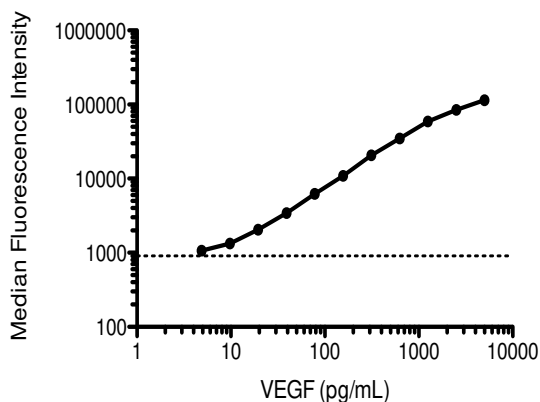

Lowest Detectable Test Conc. (pg/mL): 39.1

Lowest Detectable Test Conc. (pg/mL): 4.9

For research purposes only. Not for resale.

Rev. 1 Jan 2014